

THE INFORMATION CONTAINED IN THIS DRAWING IS THE SOLE PROPERTY OF CHILDRENS HOSPITAL BOSTON. ANY REPRODUCTION IN PART OR WHOLE WITHOUT THE WRITTEN PERMISSION OF CHILDRENS HOSPITAL BOSTON IS PROHIBITED.


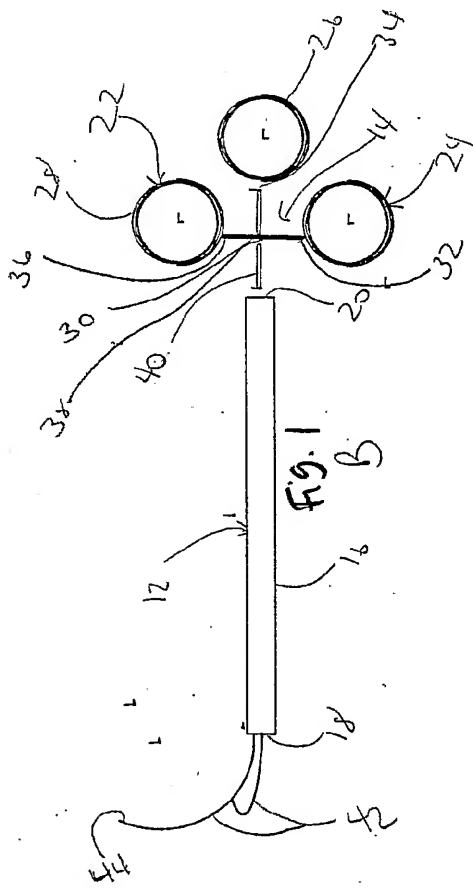


Fig. 1

Fig. 1A

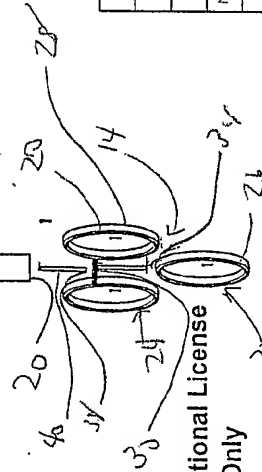

SolidWorks Educational License  
Instructional Use Only

ITEM NO.	PART OR IDENTIFYING NO.	NOMENCLATURE OR DESCRIPTION	MATERIAL SPECIFICATION	QTY REQD
PARTS LIST				
UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN CM. TOLERANCES ARE FRACTIONS DECIMALS ANGLES +/- 0.01 +/- 1		CAD GENERATED DRAWING. DO NOT MANUALLY UPDATE		
APPROVALS		DATE	CHILDRENS HOSPITAL--BOSTON	
DRAWN		JWC, MD	Patch Holder Assembly	
CHECKED		6/12/2002	SITE DWG. NO.	
MATERIAL			A	
FINISH			SCALE	
DO NOT SCALE DRAWING			CAD FILE	
NEXT ASSY			SHEET	
APPLICATION			OF	


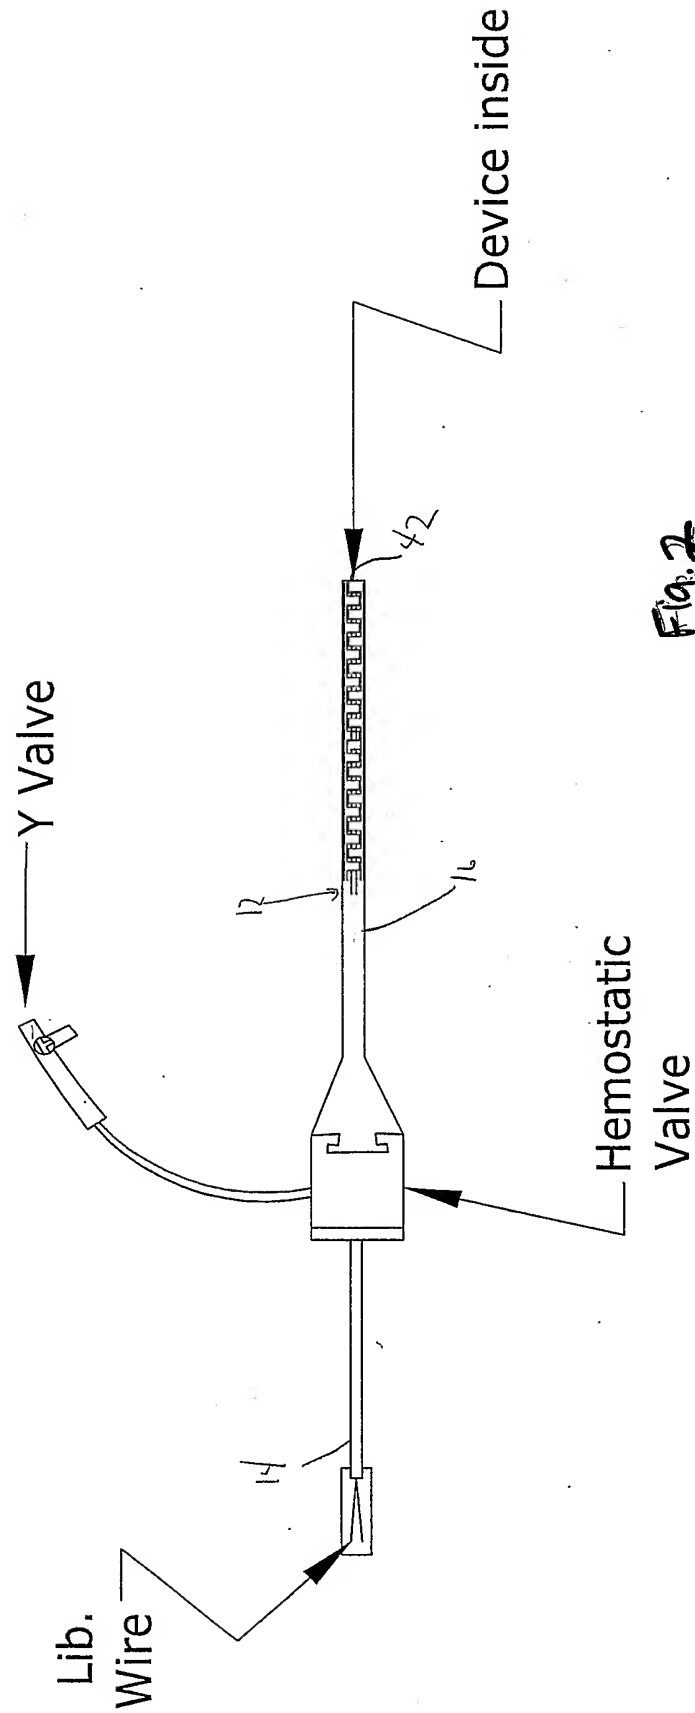


Fig. 2

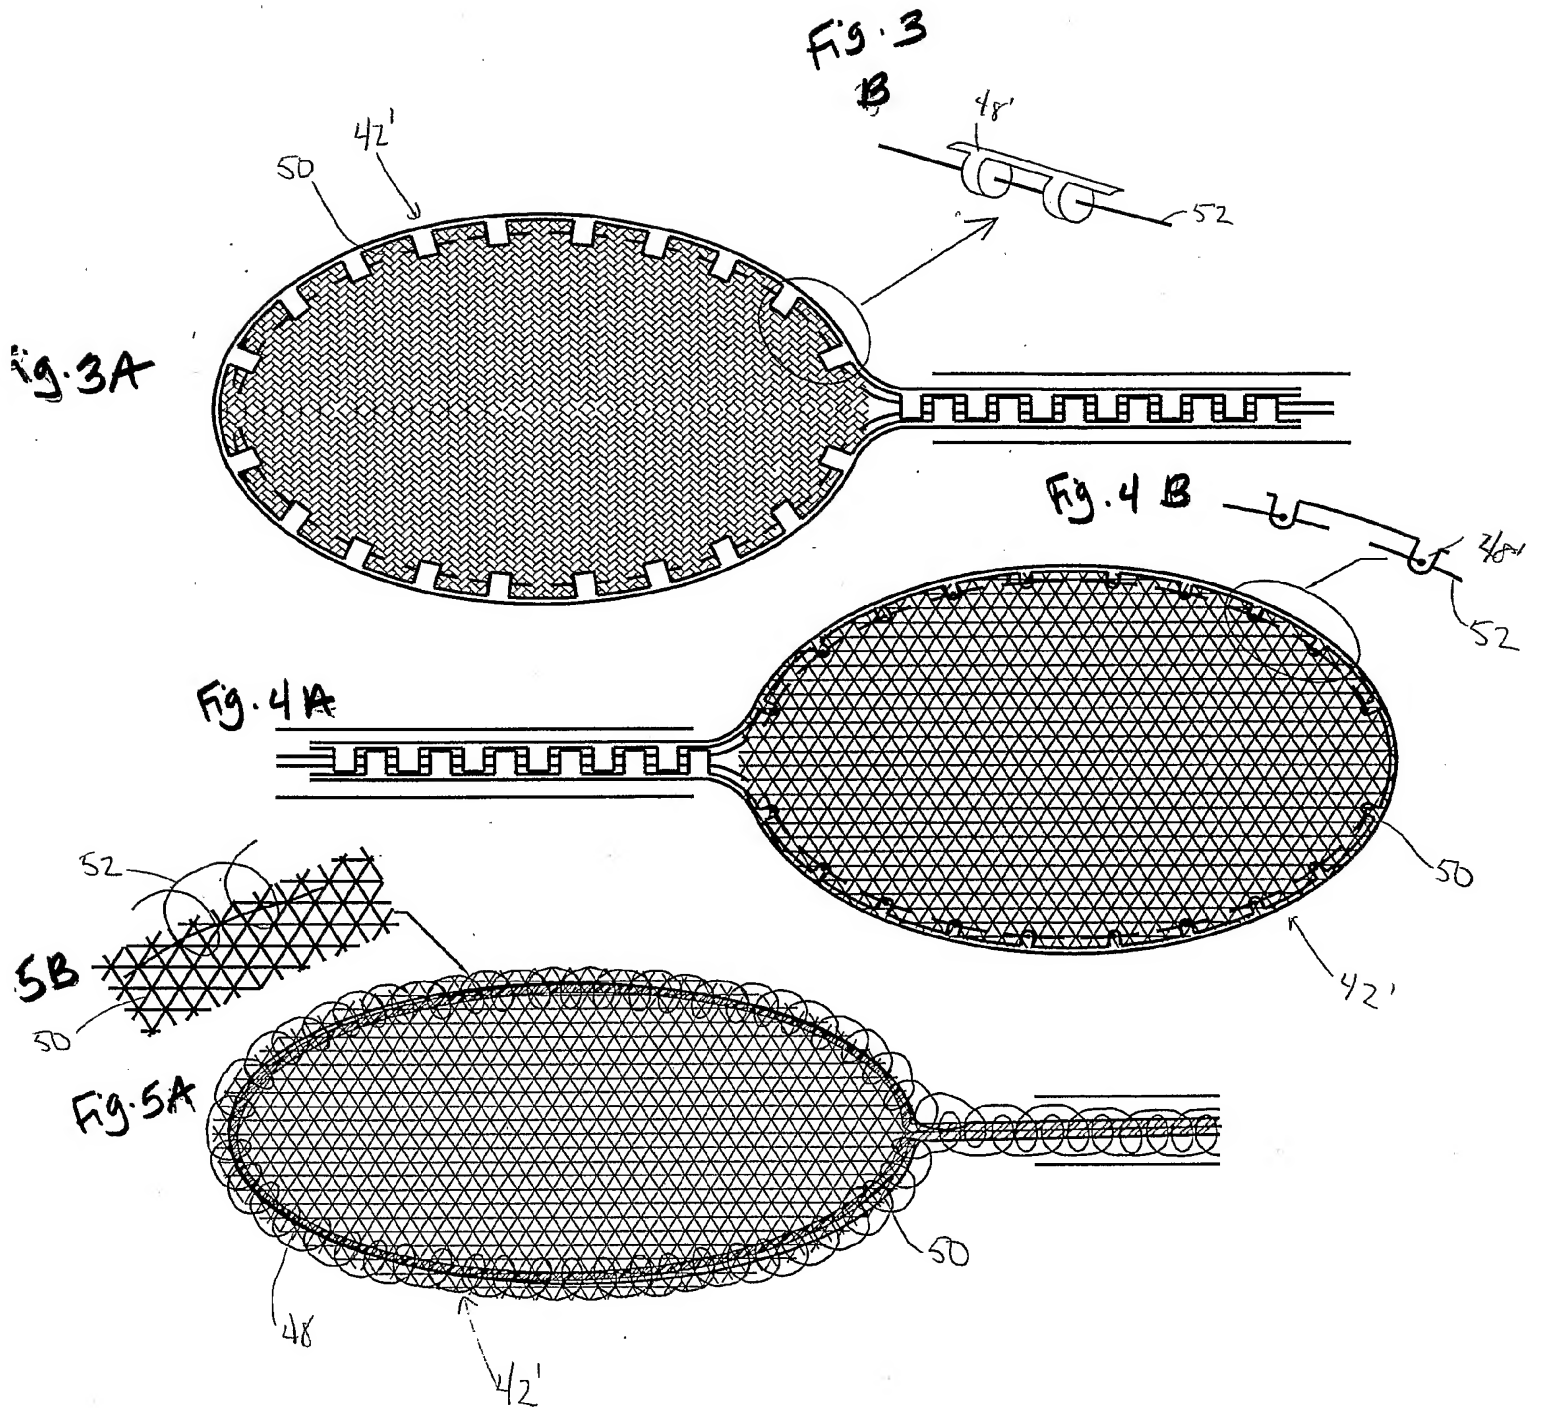

# Coil System

Fig. 6 A



Fig. 6 B

# Band System

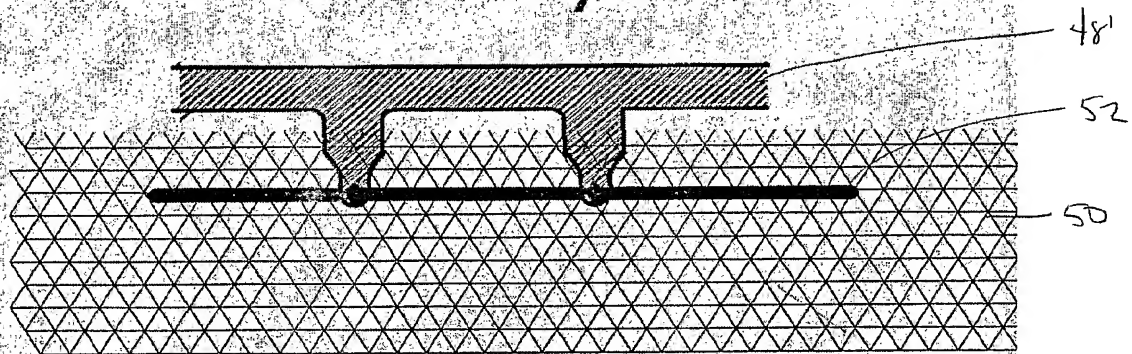


Fig. 6 C

# Tube System

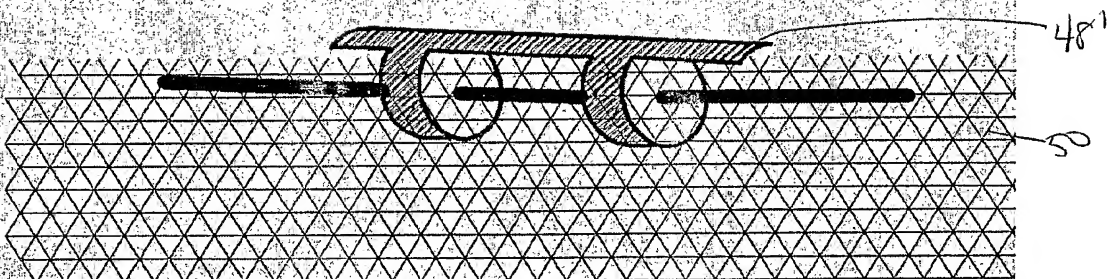


Fig. 6 D

# Mesh System



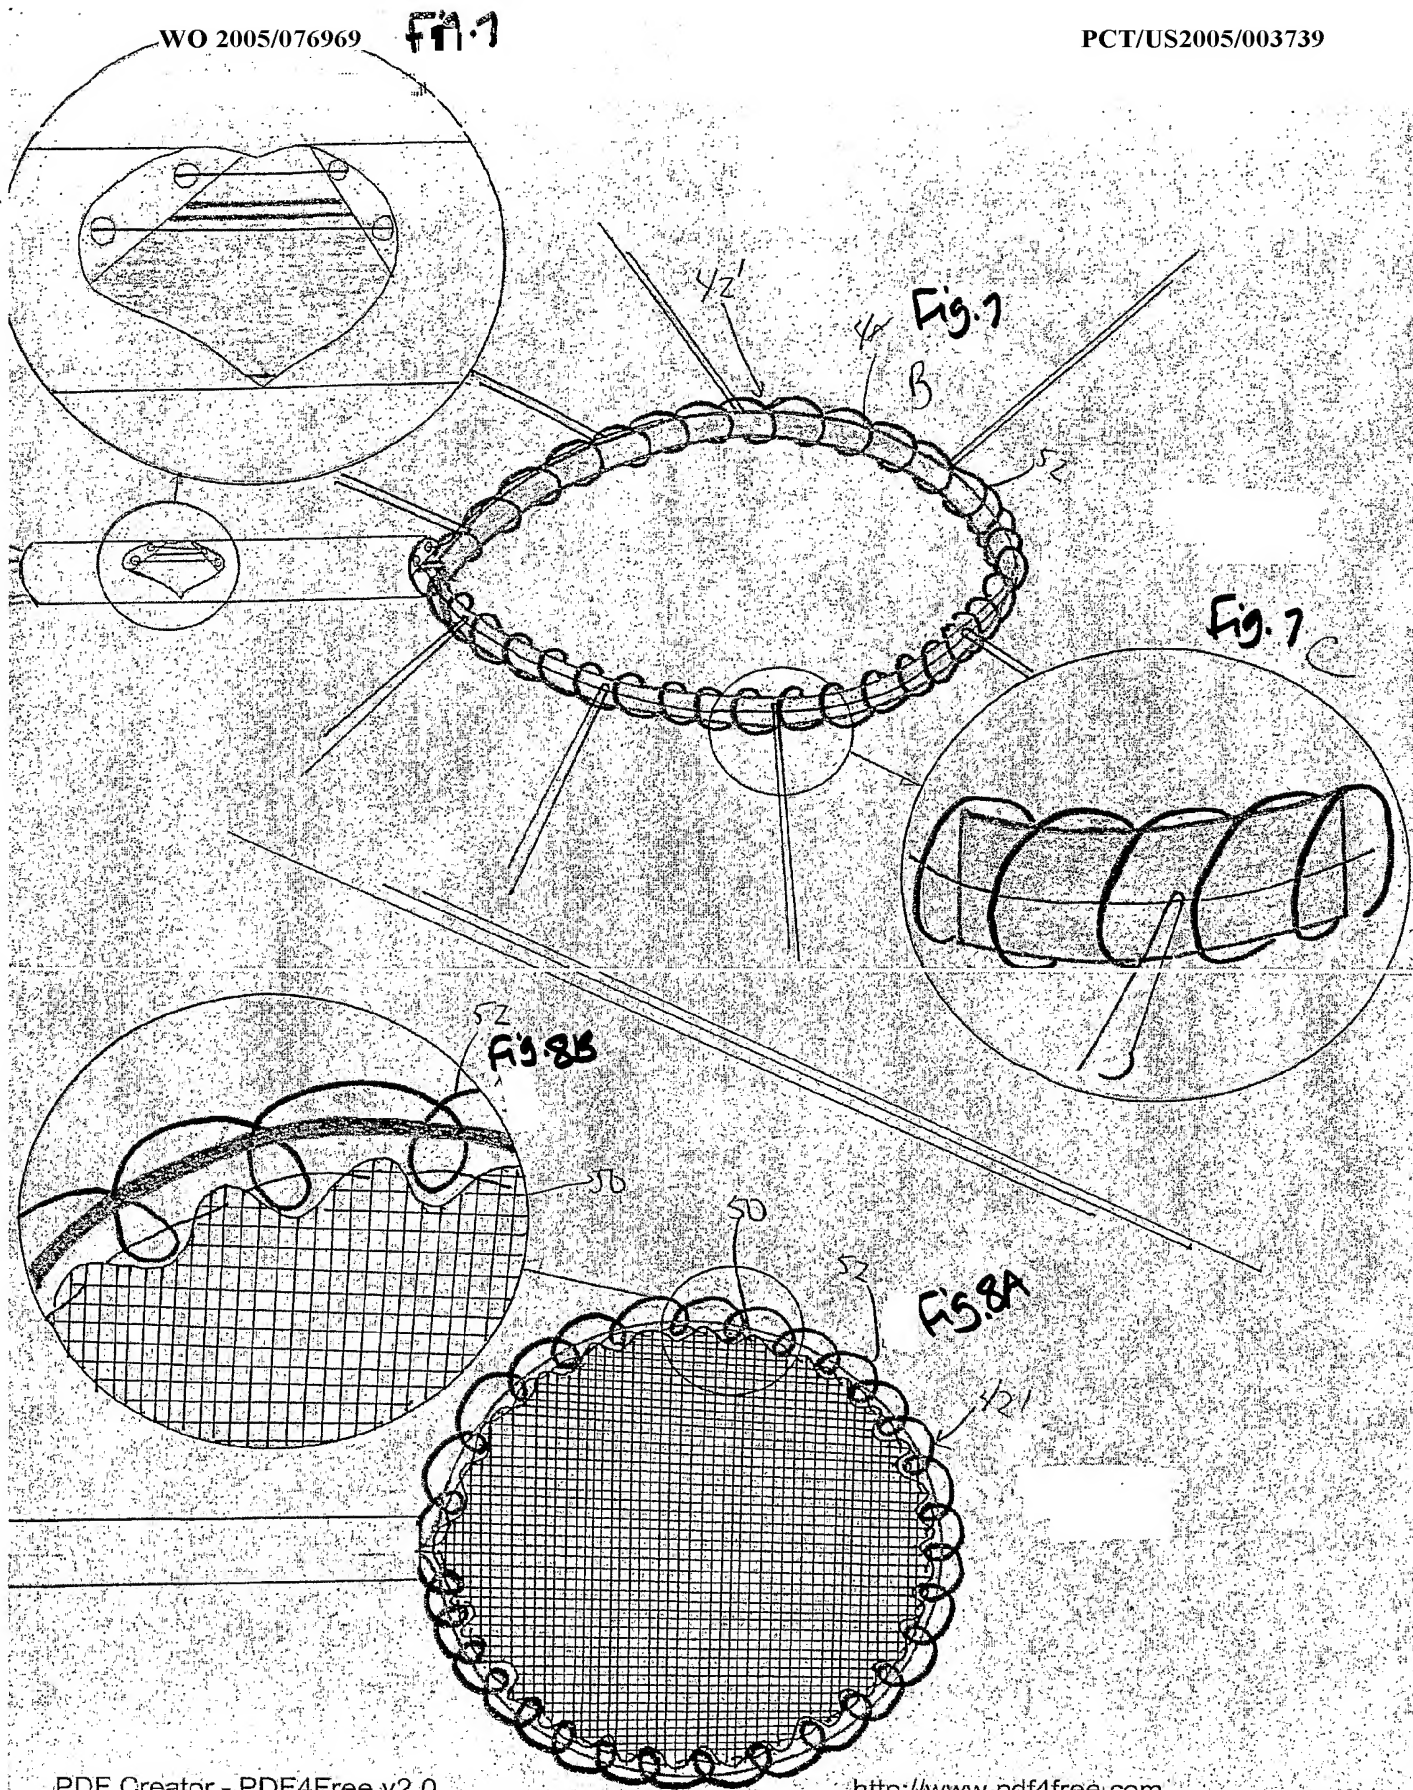
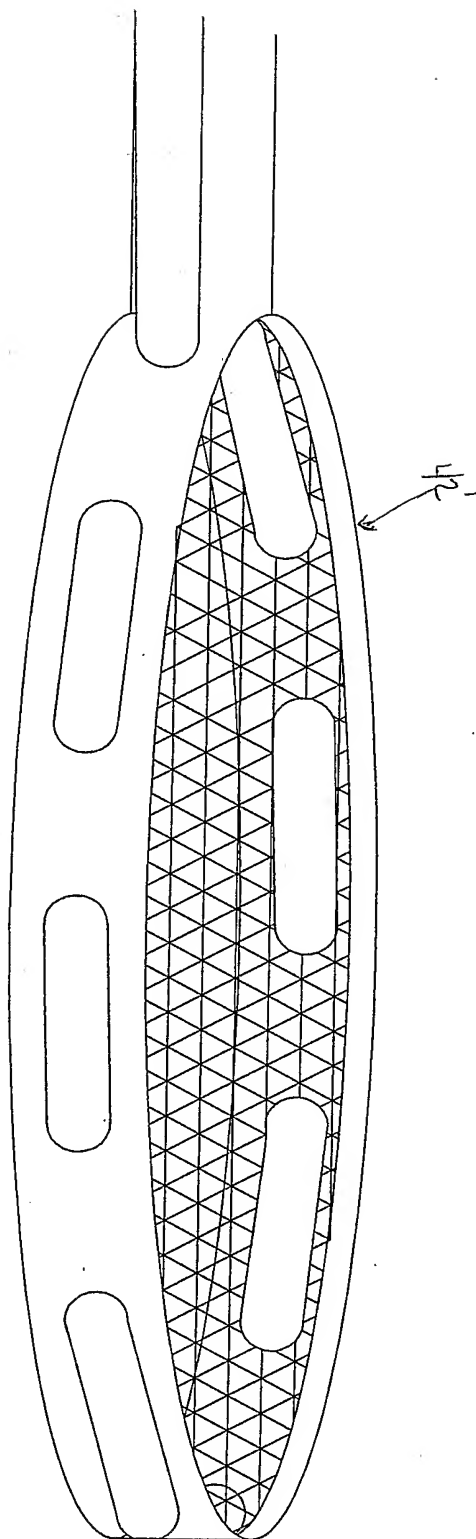
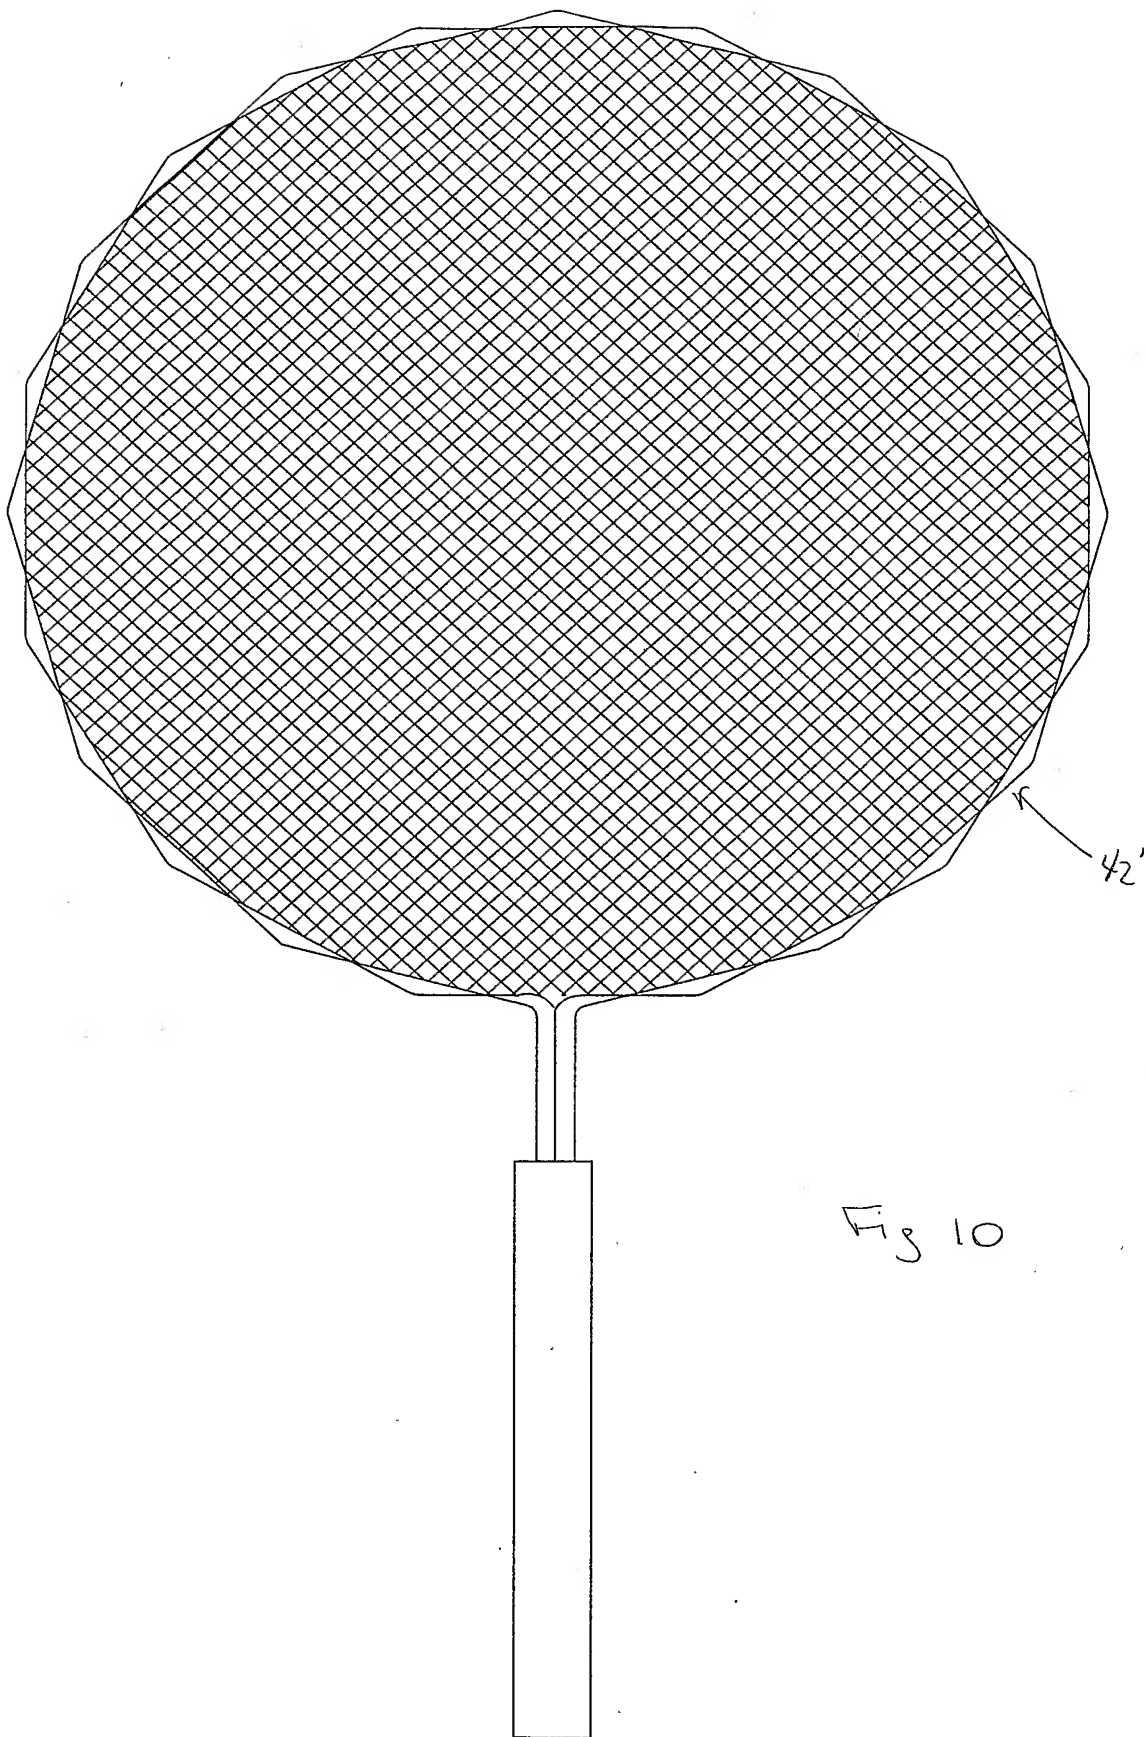


Fig 9







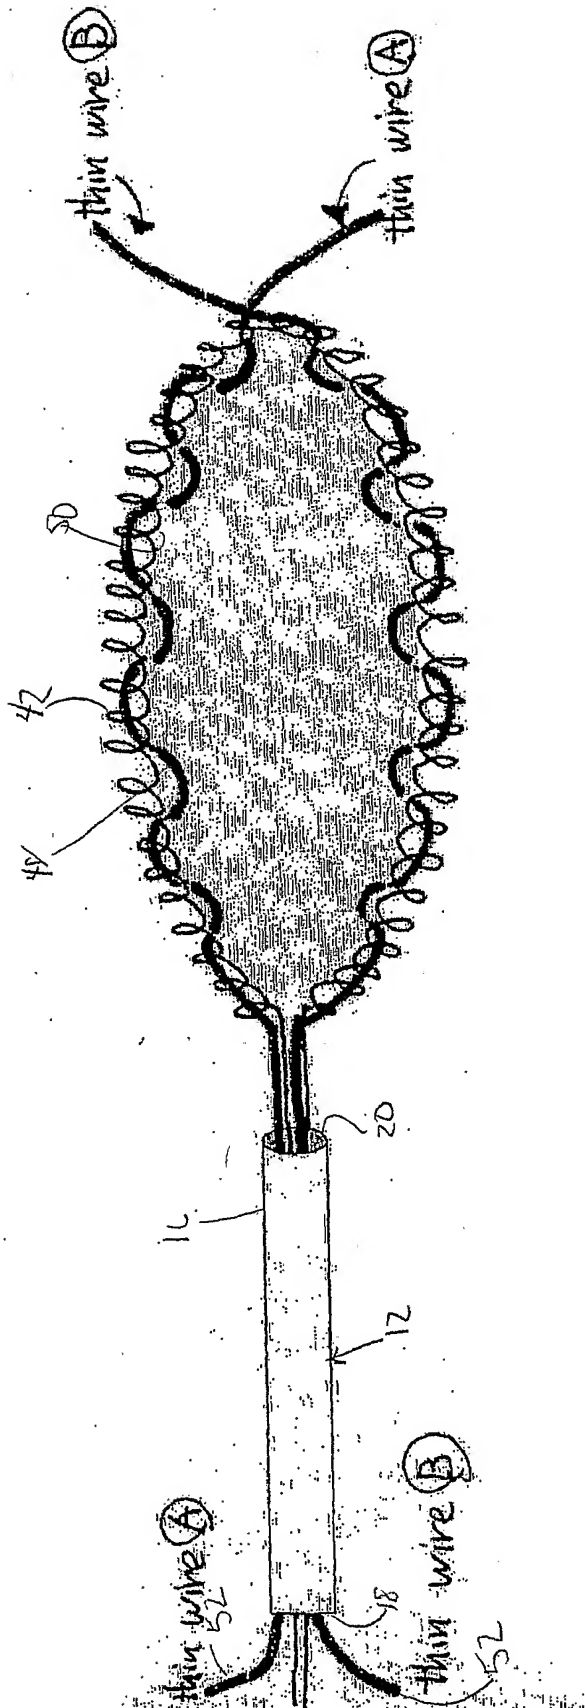
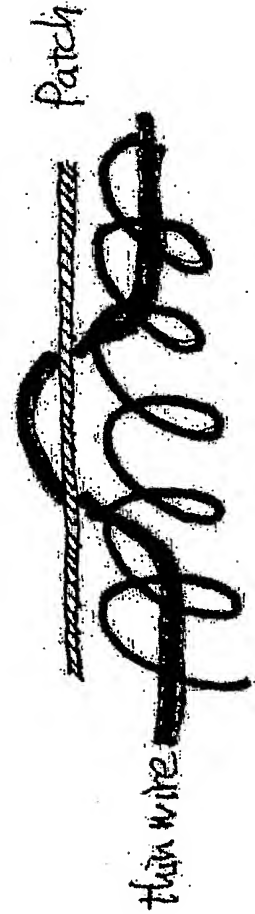


Fig. 1





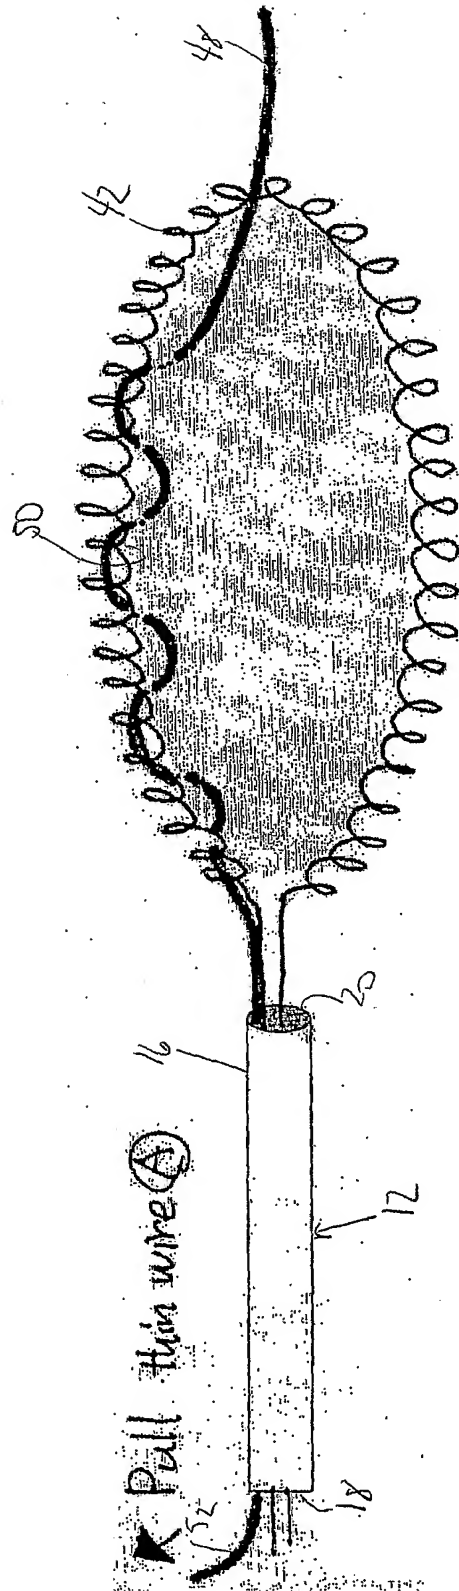


Fig. 12


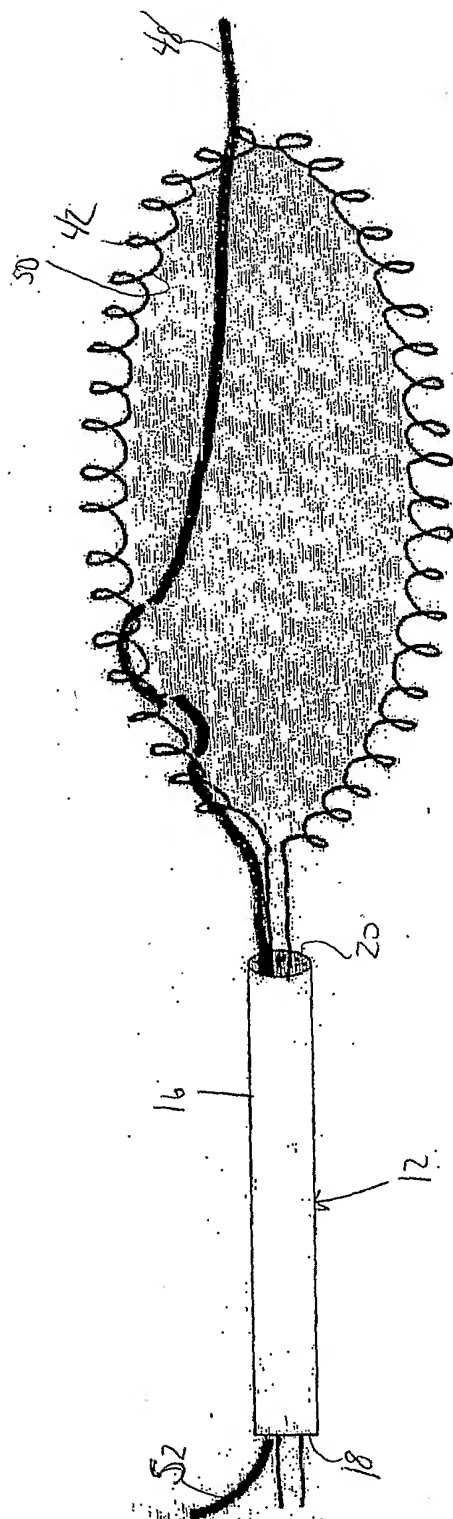


Fig. 13

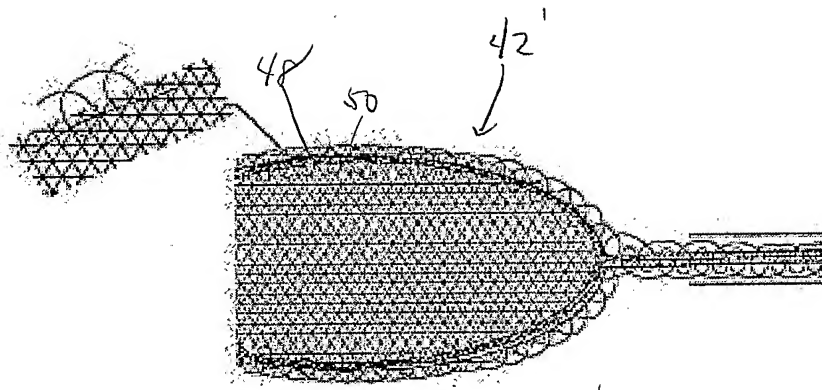

Spatula type deployment device

Fig. 14